

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

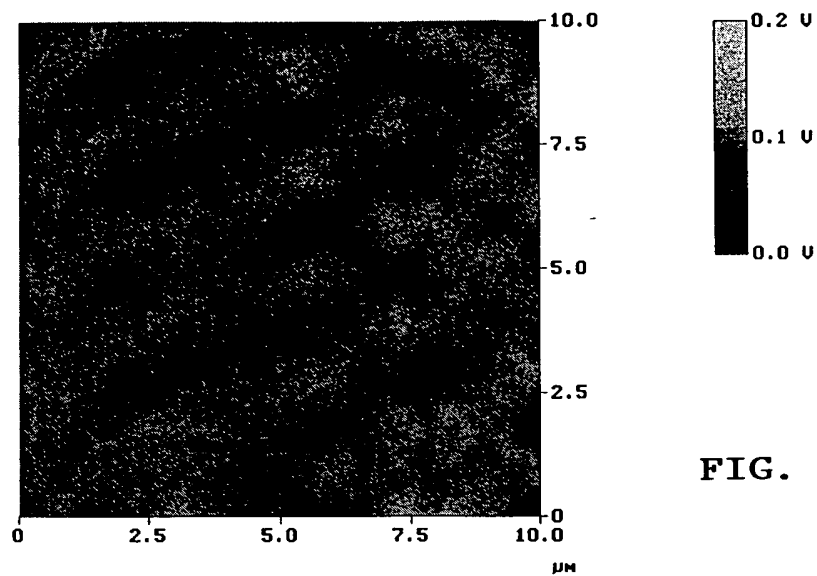


FIG. 1A

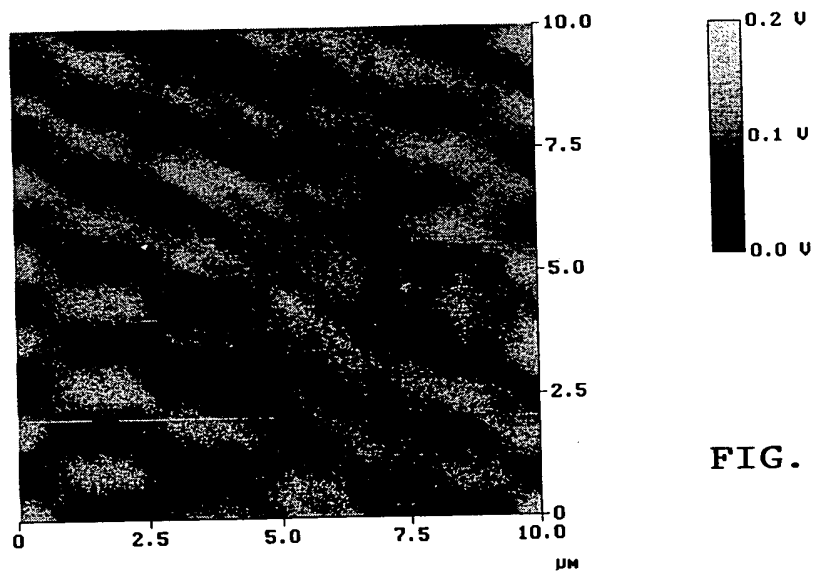


FIG. 1B

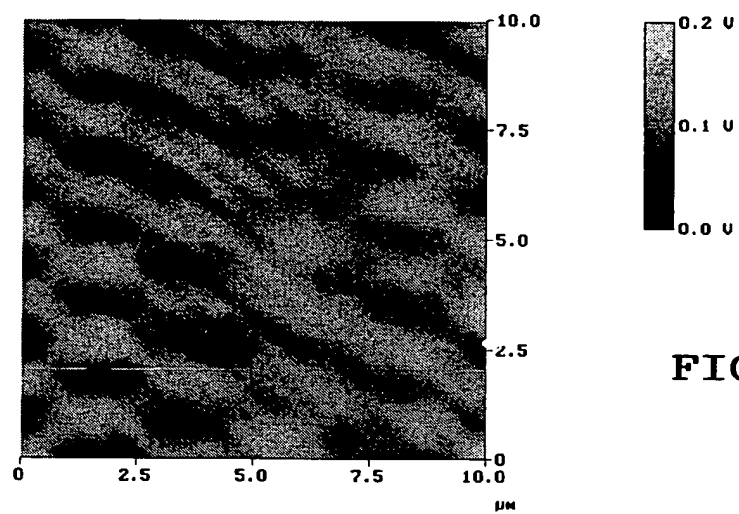


FIG. 2A


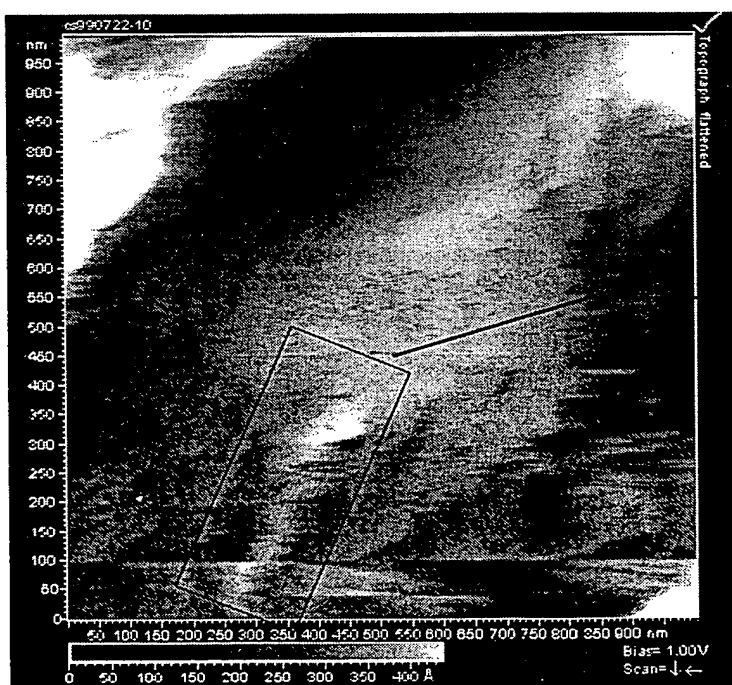





FIG. 2B

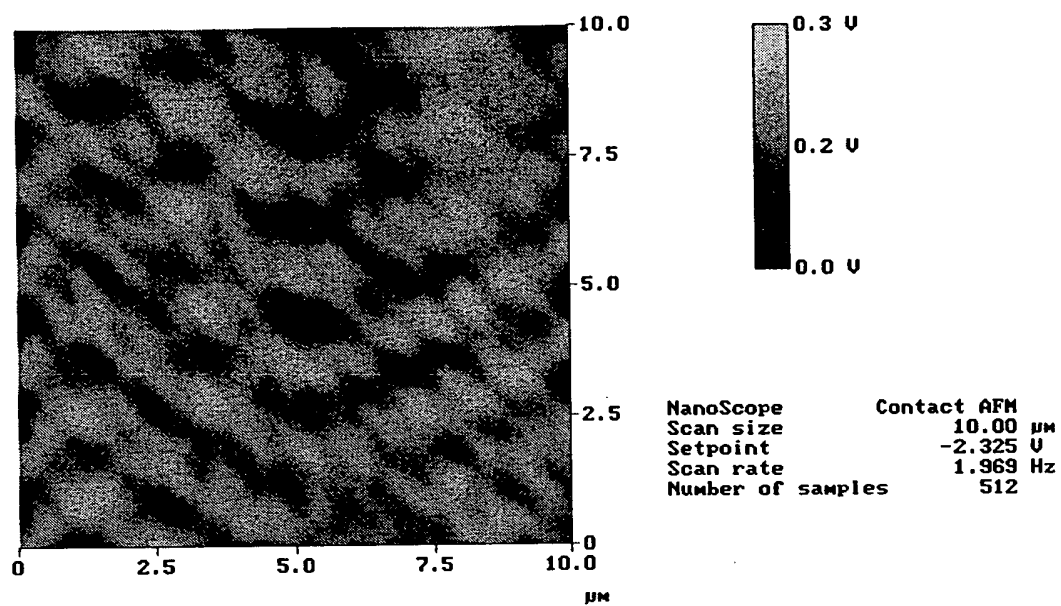

p1990722.037

MFM: Sample 231 Void Scan

FIG. 5A

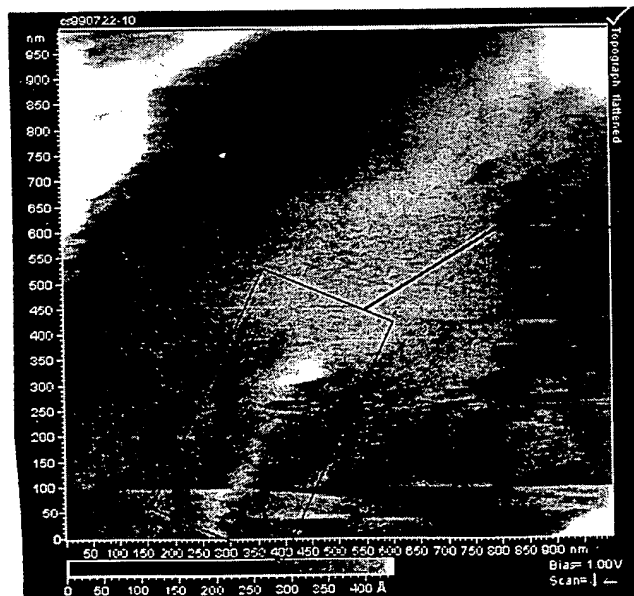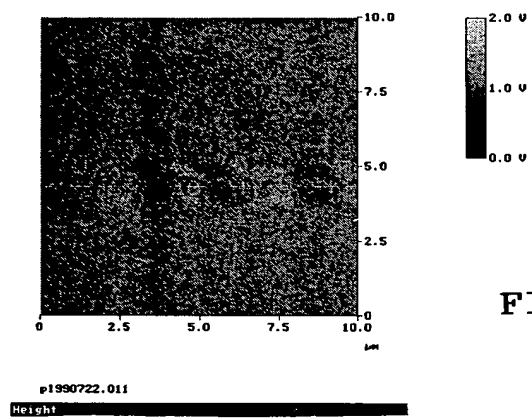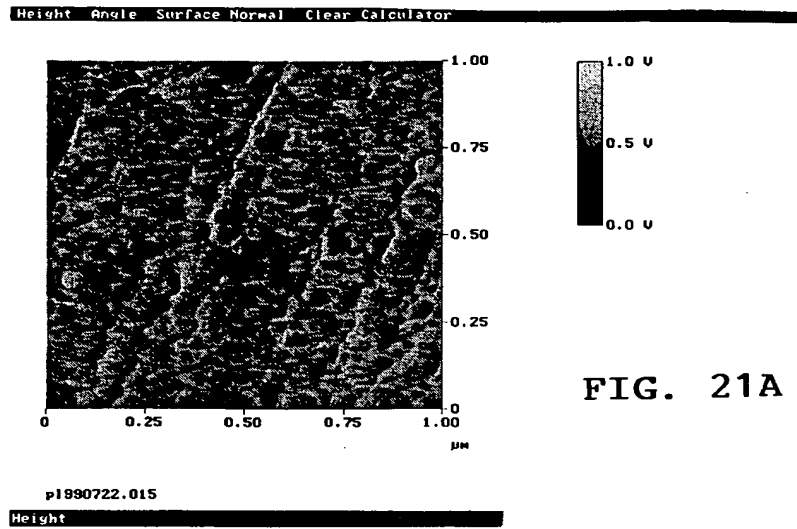

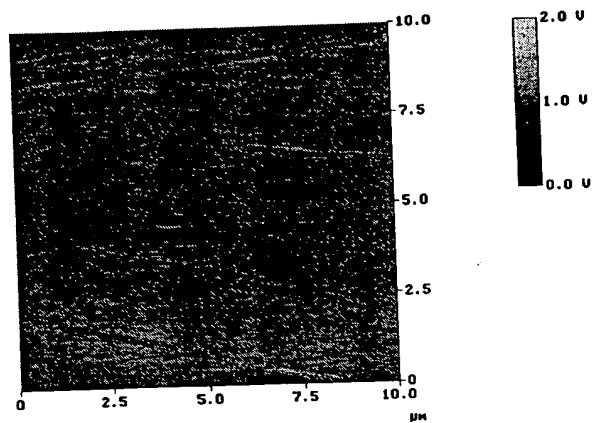


FIG. 22A

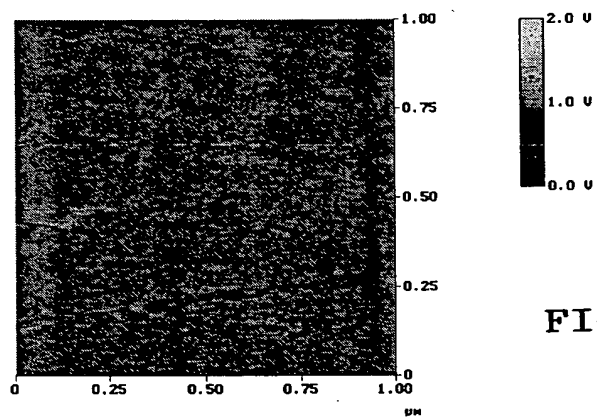


FIG. 22B


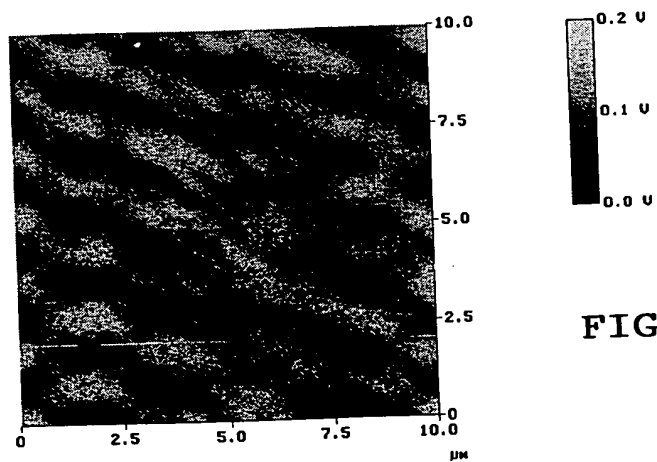


FIG. 22C

Nickel Scans: Nickel Analysis

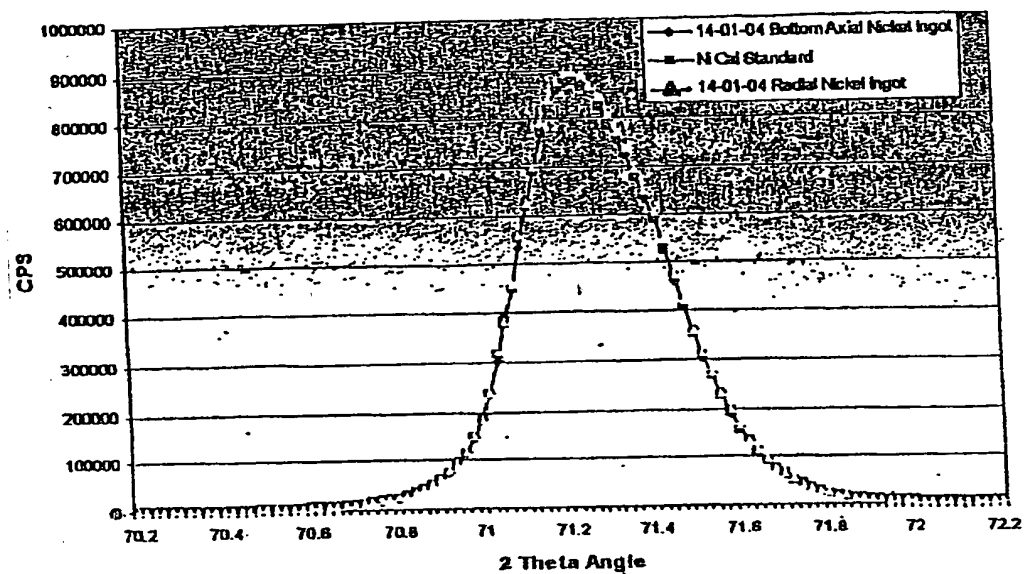

K_{α} Nickel Scans
Run 14-01-04

FIG. 27A

L_{α} Nickel Scans
Run 14-01-04


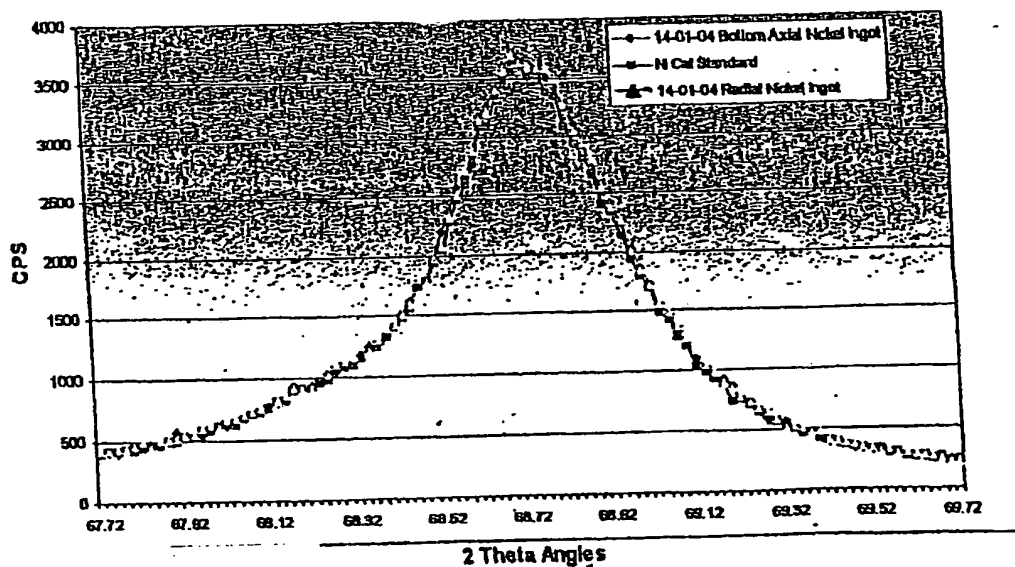


FIG. 27B

Nickel Scans: Al and Zr

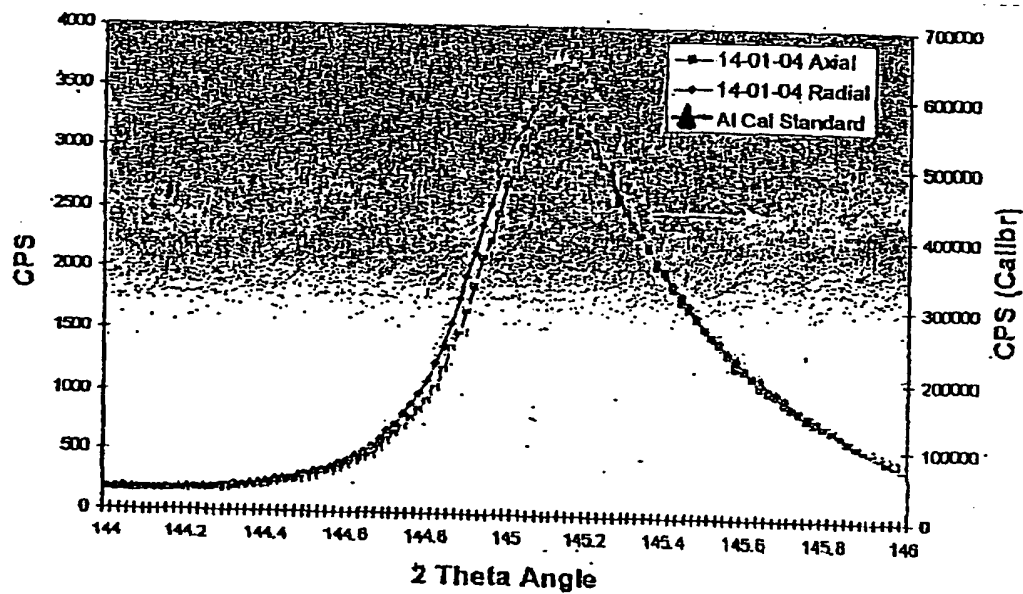

K_α Aluminum Scans of Nickel
Run 14-01-04

FIG. 28A

Nickel Scans: Cl

K_{α} Chlorine Scans of Nickel
Run 14-01-04


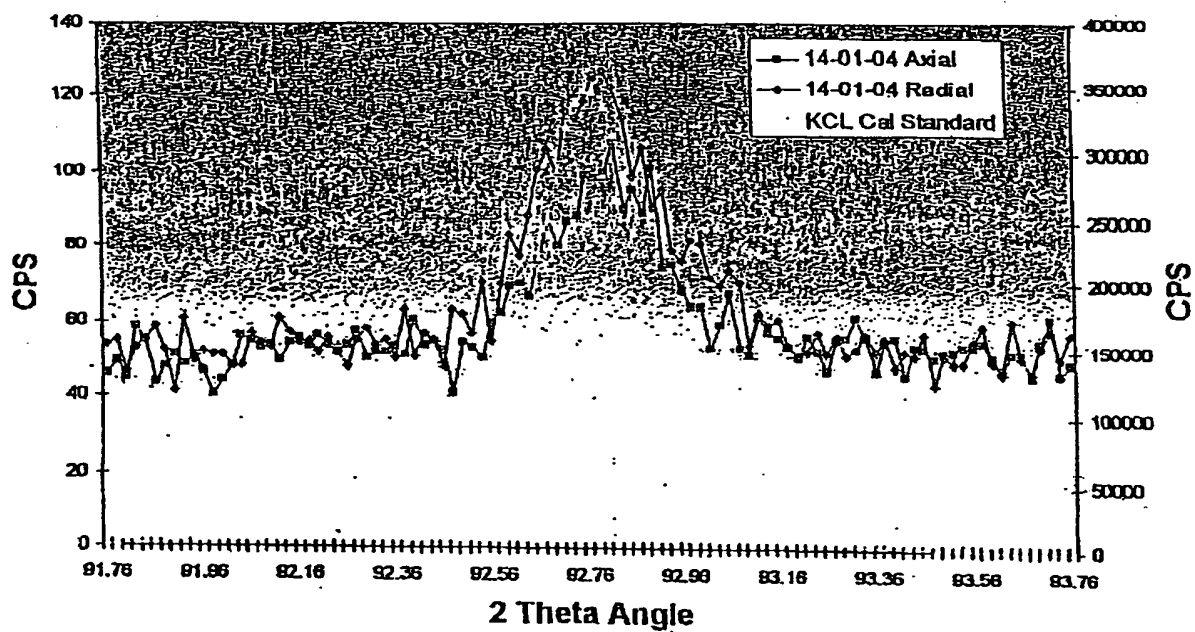


FIG. 30

Cobalt Scans: Cobalt Analysis

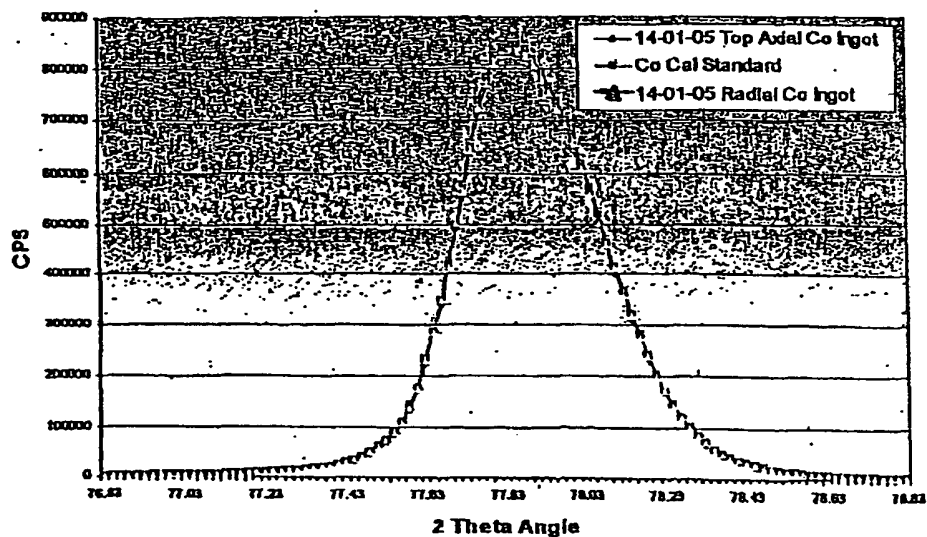

K_α Cobalt Scans
Run 14-01-05

FIG. 31A

L_α Cobalt Scans
Run 14-01-05


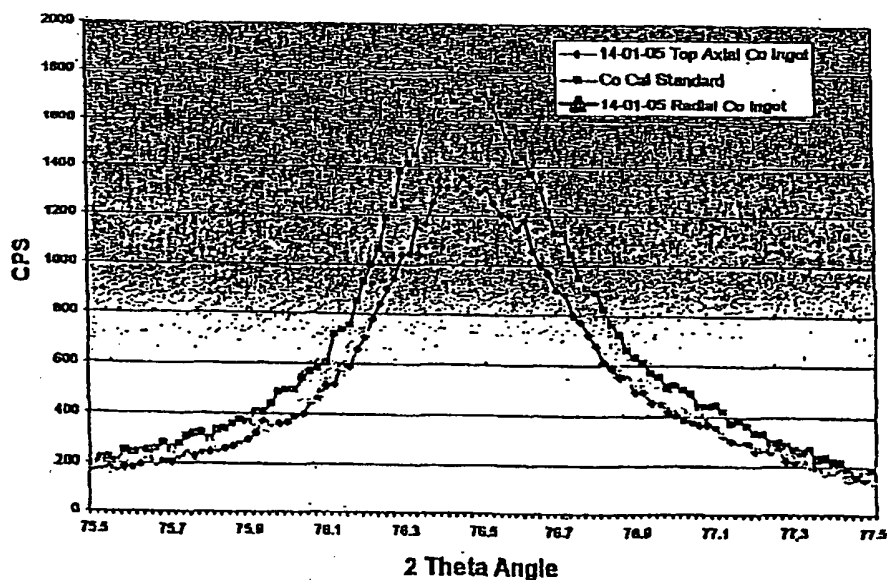


FIG. 31B


Cobalt Scans: Al and Fe

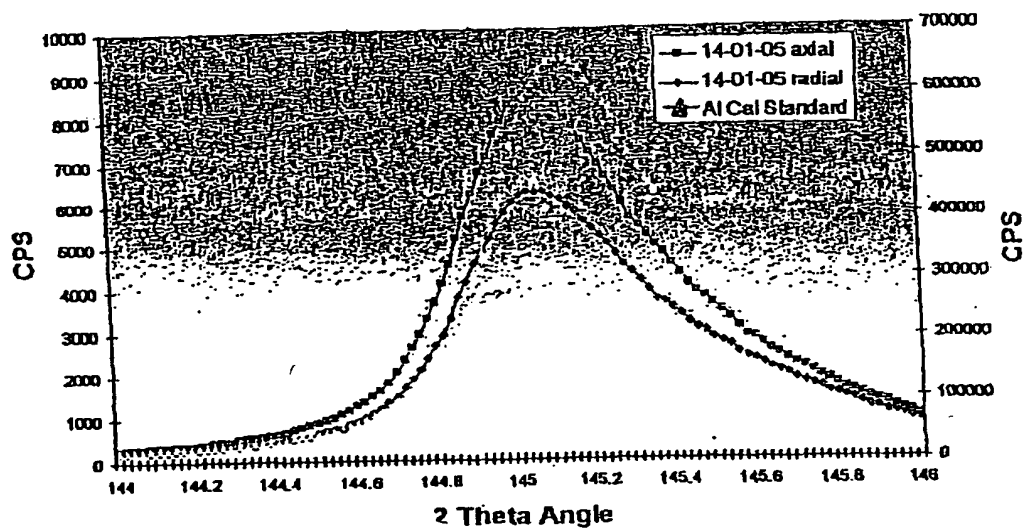

K_{α} Aluminum Scans of
Run 14-01-05

Cobalt

FIG. 32A

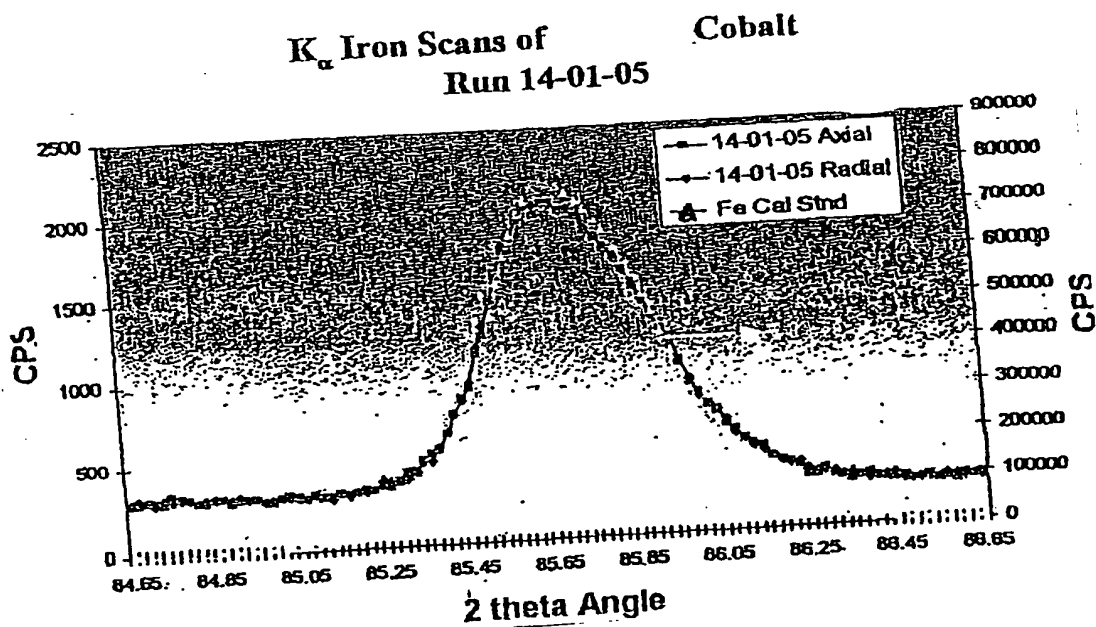


K_{α} Iron Scans of
Run 14-01-05

Cobalt

FIG. 32B


Cobalt Scans: Cl and Zr

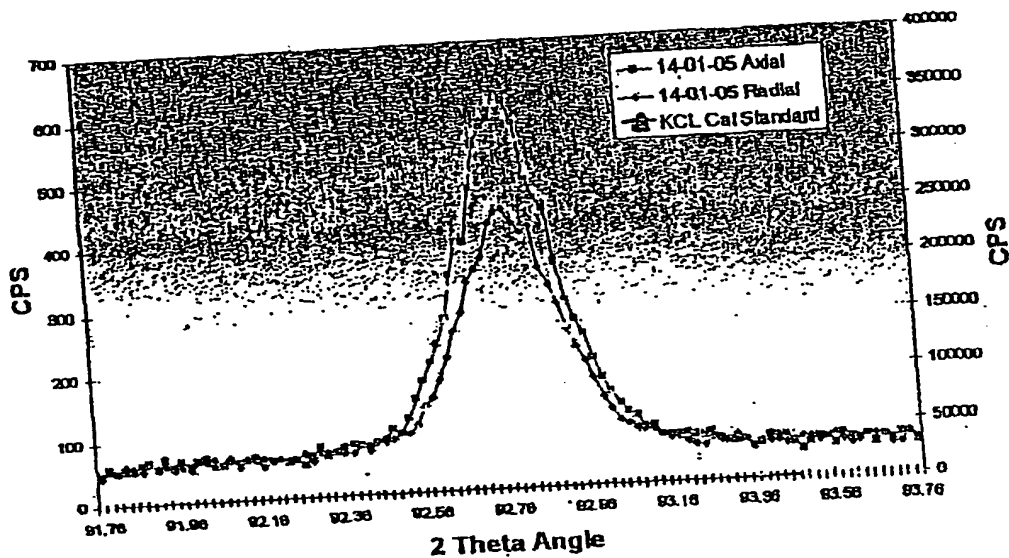

K_{α} Chlorine Scans of
Run 14-01-05

Cobalt

FIG. 33A

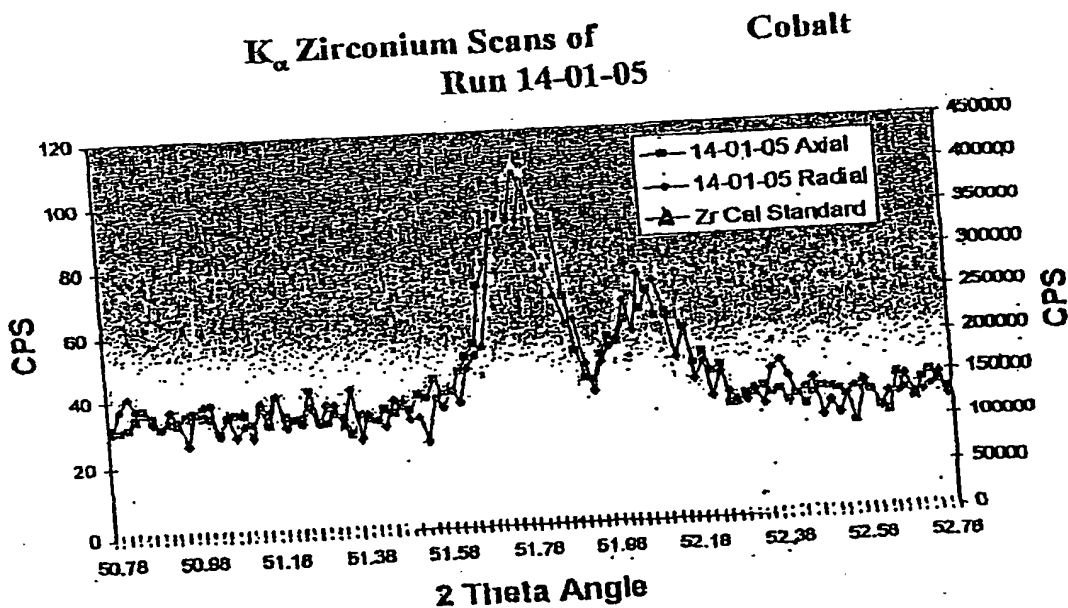


K_{α} Zirconium Scans of
Run 14-01-05

Cobalt

FIG. 33B


Cobalt Scans: Mn

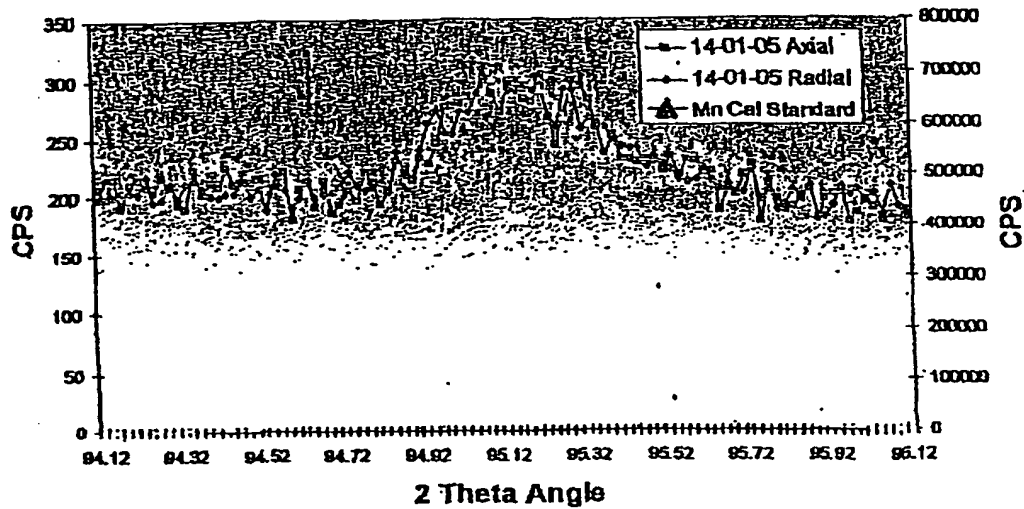

K_{α} Manganese Scans of Cobalt
Run 14-01-05

FIG. 34

Silicon Scans: Silicon Analysis

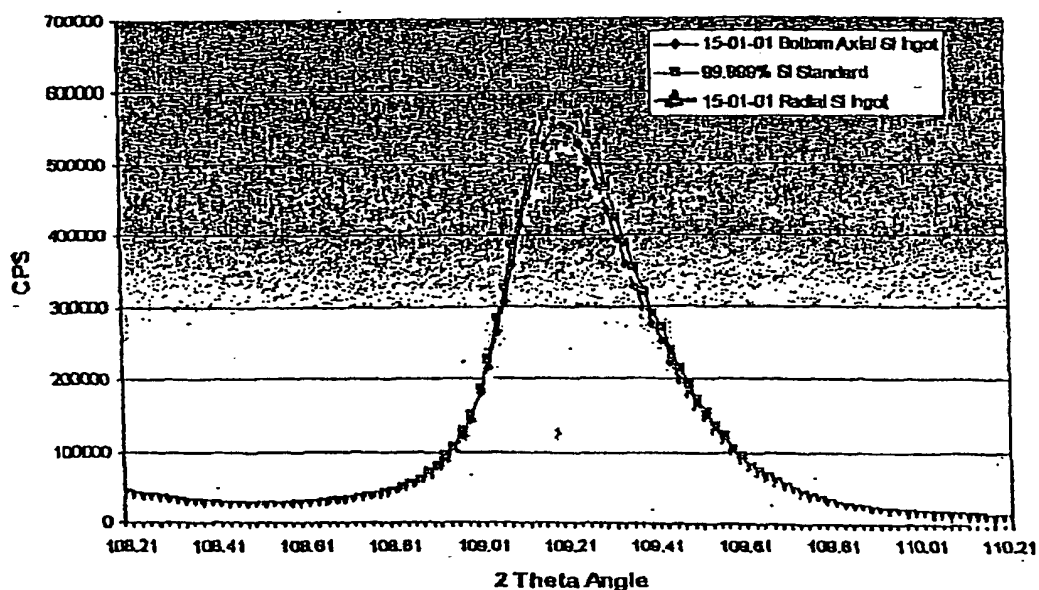

K_{α} Silicon Scans
Run 15-01-01

FIG. 45A

L_p Silicon Scans
Run 15-01-01


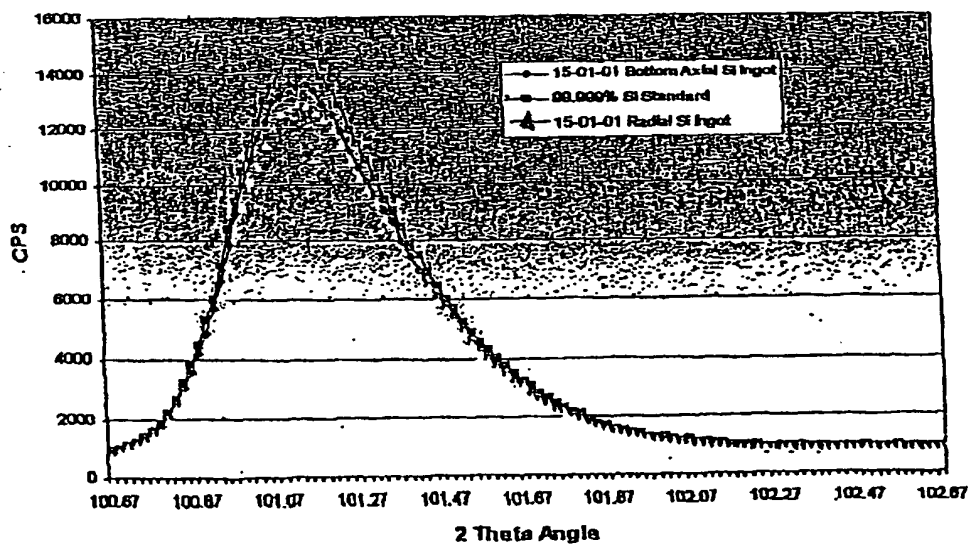



FIG. 45B

Silicon Scans: Al and Ti

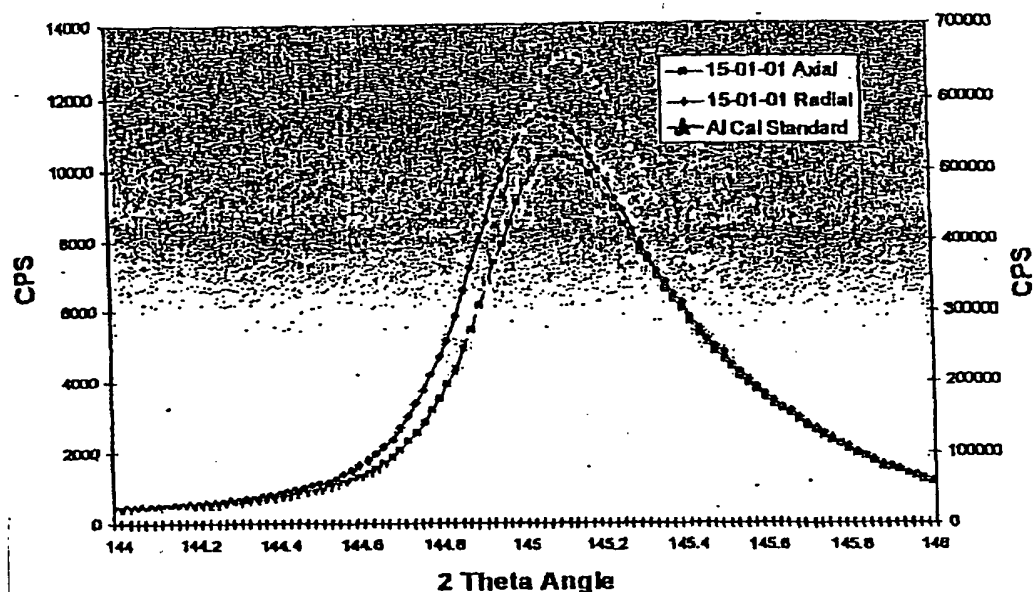

K_{α} Aluminum Scans of Silicon
Run 15-01-01

FIG. 46A

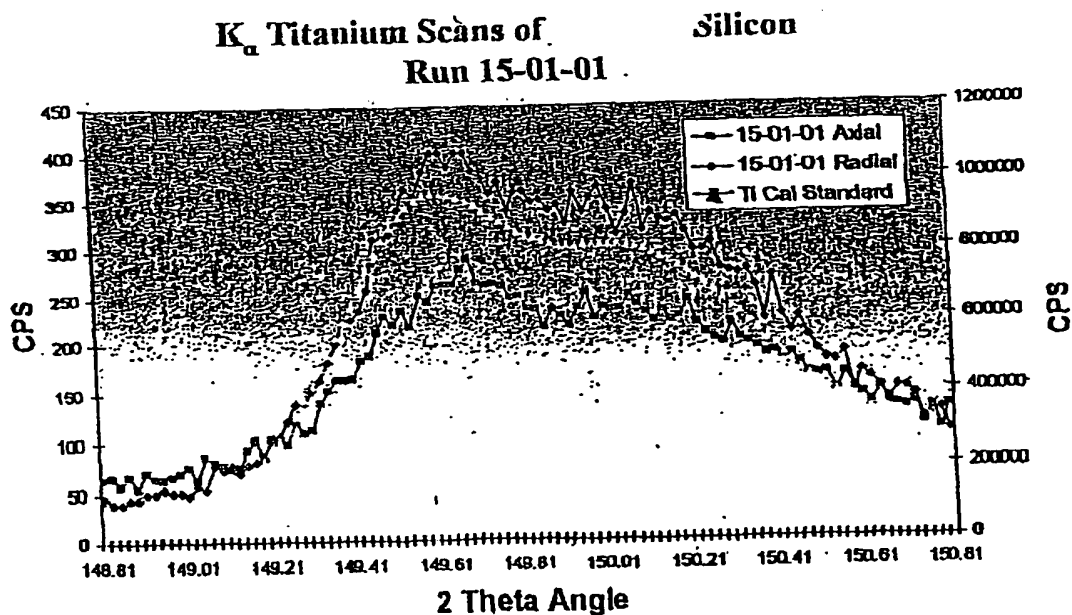

K_{α} Titanium Scans of Silicon
Run 15-01-01

FIG. 46B

Silicon Scans: S and Cl

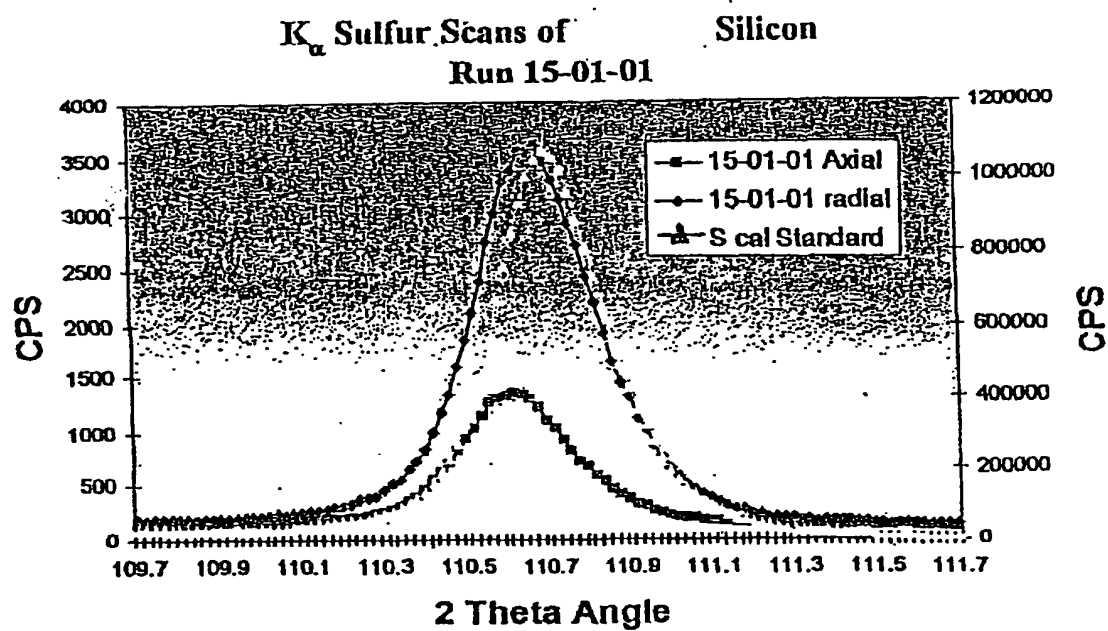


FIG. 47A

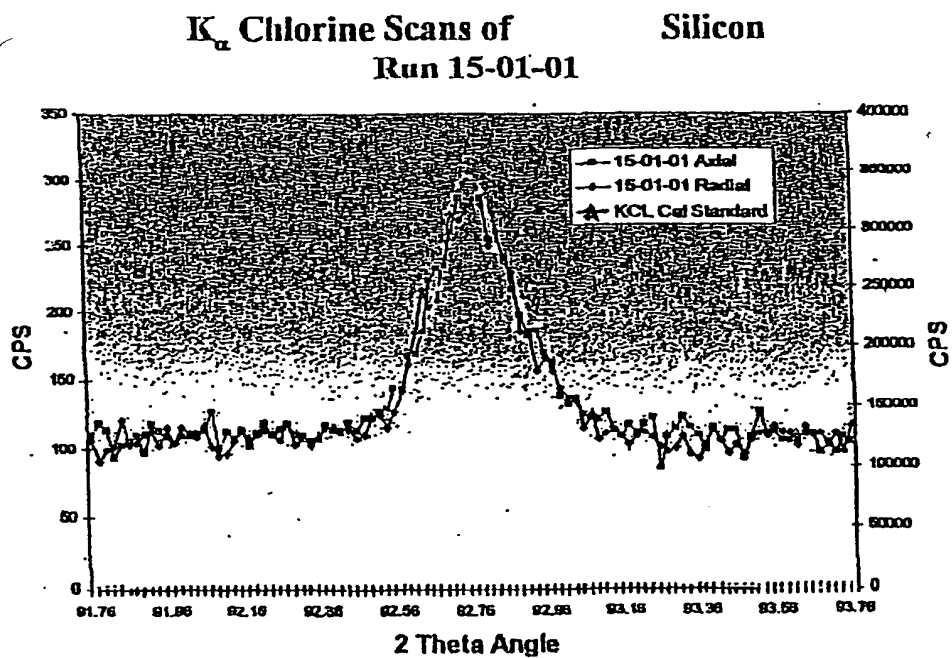


FIG. 47B

Silicon Scans: Ga and K

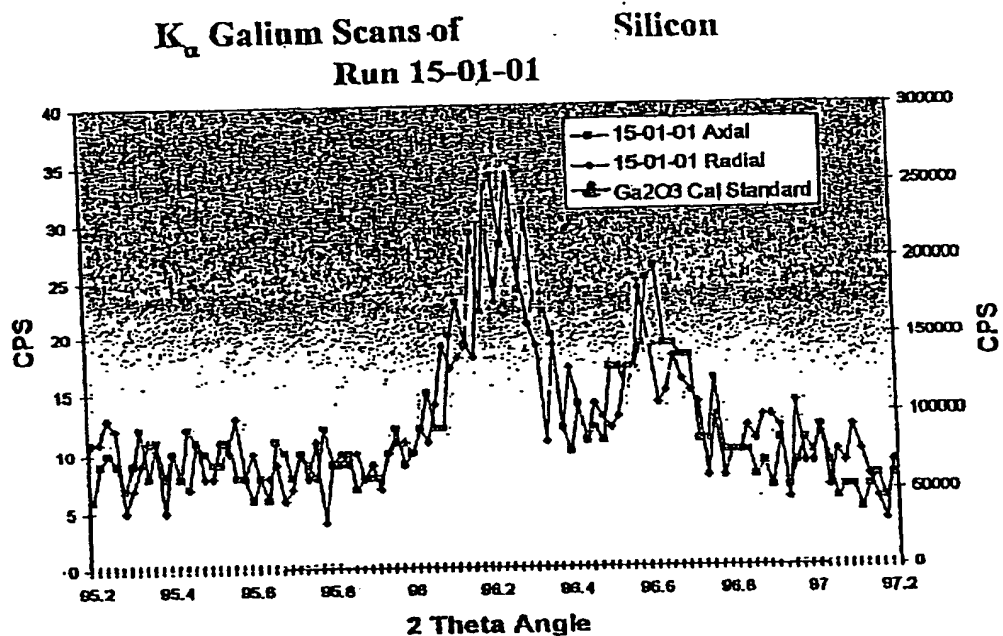


FIG. 48A


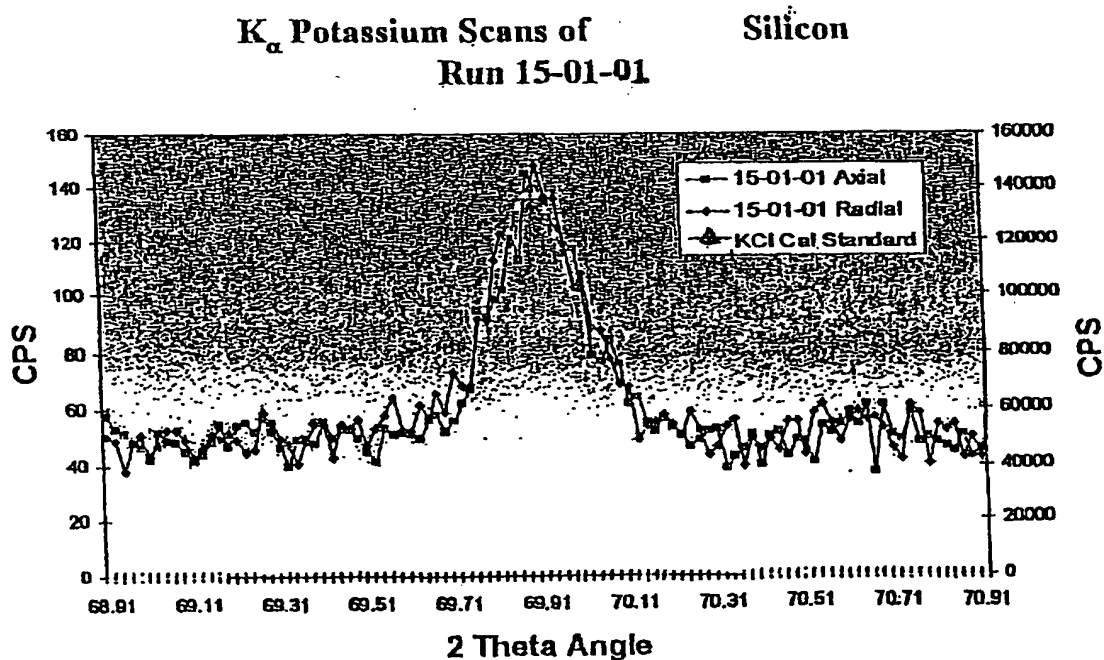


FIG. 48B

Iron Scans: Iron Analysis

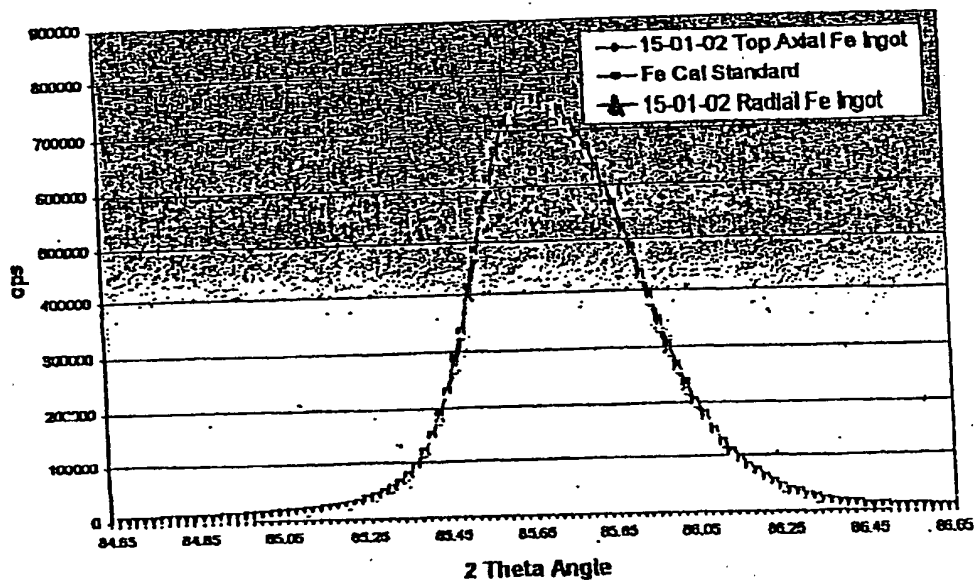

K_{α} Iron Scans of Iron
Run 15-01-02

FIG. 49A

L_{α} Iron Scans of Iron
Run 15-01-02


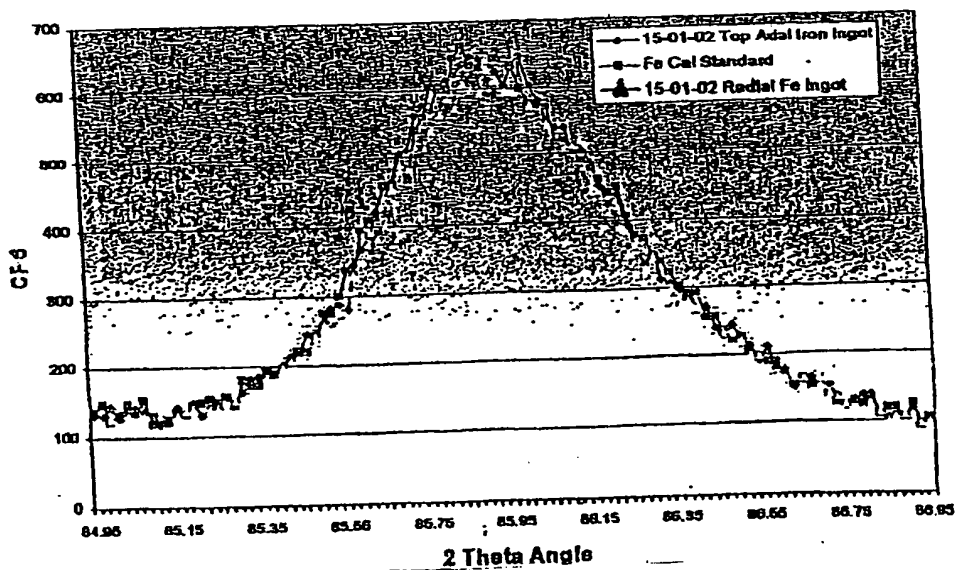


FIG. 49B

Iron Scans: Al and Zr

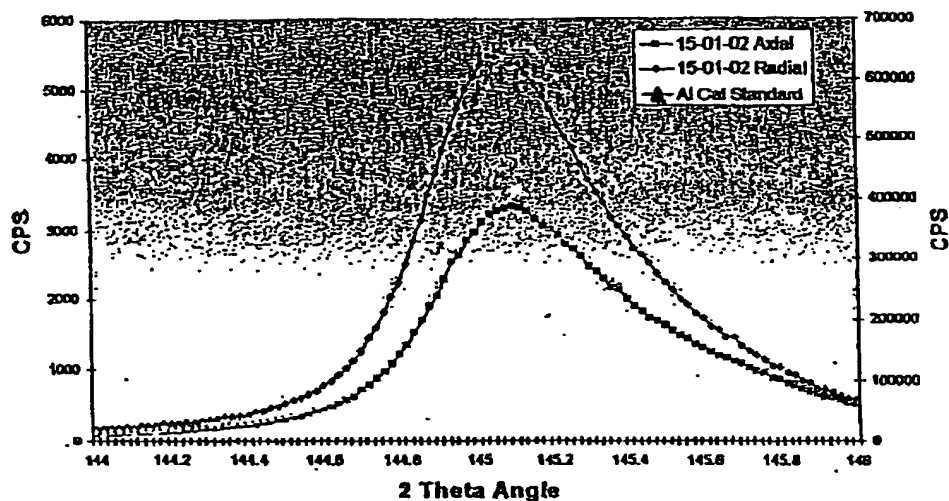

K α Aluminum Scans of Iron
Run 15-01-02

FIG. 50A

K α Zr Scans of Iron
Run 15-01-02


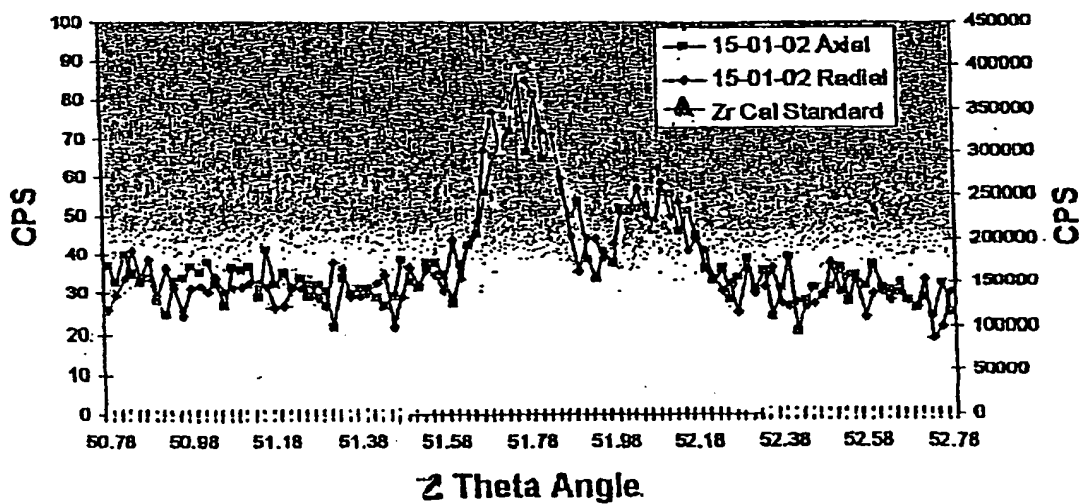


FIG. 50B

Iron Scans: S and Cl

K_{α} Sulfur Scans of Iron
Run 15-01-02

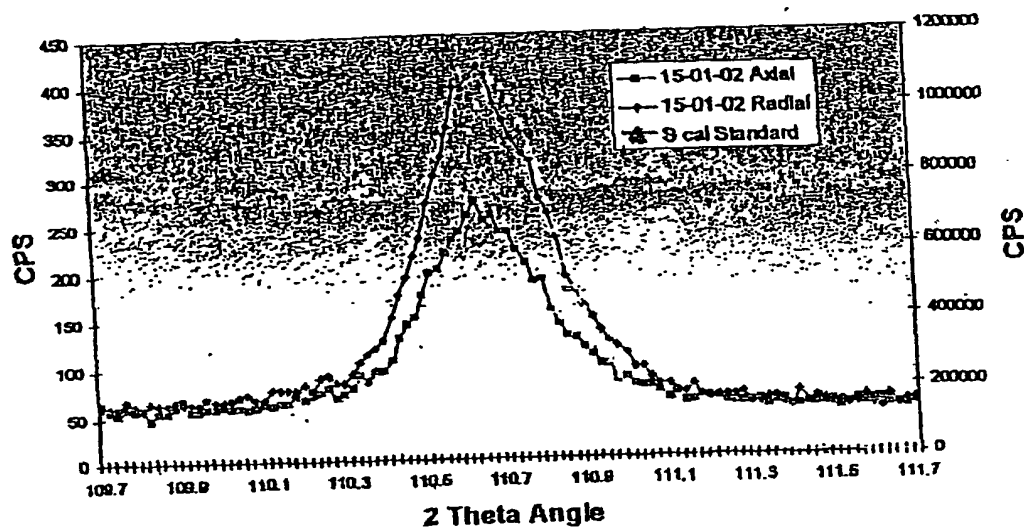

K_{α} Chlorine Scans of Iron
Run 15-01-02

